# **H8** Hemoglobin Analyzer (HPLC)

#### TECHNICAL SPECS

Methodology	High-Performance Liquid Chromatography (HPLC)
Test Modes	Variant Mode,
Test Range	3% - 18%
Precision	CV ≤1.5%
First Sample Result	7.5 Mins
Test Speed	2.2 Mins/sample for Variant Mode
Sample Type	Venous Blood, Finger Peripheral Blood, Lyophilized Whole Blood
Sample Volume	6ul, Peripheral Blood, 500ul(100 Dilution Ratio)
Auto Sample Station	10 Positions
Photometer	415nm+500nm LED, 20000 Hours Life Span
<b>Chromatography Column</b>	Available Tests ≥1500T
Filter	≥400T
Display	10.1"TFT True Color LCD Touch Screen
Software	Embedded System with Self-Diagnosis to Monitor and Detect System Errors
Reagent Kit	Eluent A, Eluent B, Eluent C, Hemolysin, Calibrator, QC Material (Weight Sensor±1%)
Information Input	Scanner or Touch Keypad
Storage	20000 Sample Results
Connection	USB, LAN, LIS Compatible
Printer	Thermal Printer and External Laser Printer
Operation	Temperature 10~30°C (~°F)
Humidity	≤85%
Power	AC 100-240V 50/60HZ 120VA
Dimensions	580mm×500mm×520mm (22.8"H×19.7"W×20.5"D)
Weight	50kg (110lbs)
Barcode Scanner	External















E-mail: matrixlabschennai@gmail.com Phone: 044-2624 4545 / 43852222 Toll Free: 18001201713





**H8** Hemoglobin Analyzer (HPLC)

# **H8** Hemoglobin Analyzer (HPLC)



The Fully automated Lifotronic H8 Hemoglobin Analyzer offers the fast throughput of HbA1c results in 1.2 miuntes, with Hb variant detection, providing the outstanding solution for quick and reliable diabetic monitoring. No sample preparation and very little hands-on time by the operator is required for the H8 Analyzer.






#### **Gold Standard of Diabetes Diagnose**

Glycosylated hemoglobin (HbA1c) is widely recognized as a Gold Standard to monitor diabetes, which can indicate the average plasma glucose concentration over 8~12 weeks.

### **HPLC Methodology**

High-PressureLiquid Chromatography (HPLC), to separate HbA1c directly with measuring the absorbance points continually to form chromatogram. Using normal distribution curve fitting algorithm to get precise HbA1c testing result, excluding interference of variant and unstable hemoglobin like HbF. Standard Analysis Mode will report HbA1a、HbA1b、HbF、HbA1c、P3、HbA0 peak areas and ratio. And the result also includes IFCC, NGSP and ADAG value for diverse client needs.




12
10
8
6
4
Low Level
High Level

1 2 3 4 5 6 7 8 9 10

Correlation between H8 and a famous HPLC method

Precision Study

## The Elements of Hemoglobin

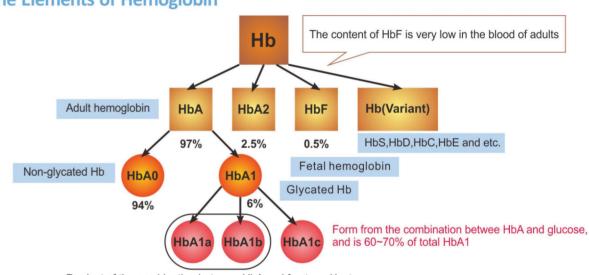

Product of the combination between HbA and fructose / lactose

# **HPLC Technology – Gold Standard Methodology**

- NGSP and IFCC certified
- HbA1c results in 2.2minutes

### **Fully Automated - To Minimize Operation Hassles**


- Primary Tube Sampling with Cap Piercing
- Fully Automated Start-up, Maintenanceand Shutdown
- Barcode Scanner for Sample identification

#### Precise and Reliable – To Serve You Consistently

- HbA1c Inter & Intra Measuring CV's ≤1.5% to EnableExceptional ResultManagement
- SuperiorQuality Chromatographic Resolution to EliminateInterferences

#### **Compact Size - To Minimize Space Requirements**

Small Footprint Reduces Bench Space Needed



en.lifotronic.com